

Northwest
Life Science Specialties, LLC

Premier Products for Superior Life Science Research

NWLSSTTM
Human IL-12p70
ELISA

Product NWK-IL12H01
For Research Use Only

***ELISA kit for quantification of the cytokine interleukin 12
(IL-12) in human biological samples.***

Table of Contents

Section	Page
Introduction	3
Intended Use	3
Test Principle	3
Specifications	4
Kit Contents	4
Required Materials Not Provided	4
Required Instrumentation	5
Warnings, Precautions, Limitations	5
Storage Instructions	5
Assay Preparation	5
Reagent Preparation	6
Sample Handling/Preparation	7
Standard Curve Preparation	7
Assay Protocol	8
Data Analysis	10
Performance Details	11
References	11
Statement of Limited Warranty	12
Notes	12

Introduction:

Interleukin-12 (IL-12p70) is a cytokine comprised of two disulfide-linked proteins (p35 and p40) and is essential for the initiation of effective immune response. The IL-12p70 heterodimer is an important cytokine secreted by antigen-presenting cells in response to antigenic stimulation. Functional IL-12p70 acts as a pro-inflammatory cytokine to stimulate T-cells and natural killer (NK) cells to produce gamma interferon (IFN-gamma). The standard product used in this kit is recombinant human IL-12p70 with a molecular mass of 75 KDa.

Intended Use:

The NWLSS™ Human IL-12p70 ELISA kit is intended to be used for the in vitro quantitative determination of the interleukin-12 heterodimer IL-12p70 in human serum, plasma, cell lysates and cell culture supernatants. The assay will recognize native and recombinant human IL-12p70.

Test Principle:

The NWLSS™ Human IL-12p70 ELISA is a sandwich format Enzyme-Linked Immunosorbent Assay (ELISA). The microtiter plate provided in this kit has been pre-coated with a monoclonal antibody specific to human IL-12p70. Samples are pipetted into these wells. Non-bound IL-12p70 and other components of the sample are removed by washing, after which a biotinylated antibody specific to human IL-12p70 is added. In order to quantitatively determine the amount of IL-12p70 present in the sample, Streptavidin Horse-radish Peroxidase (HRP) conjugate is added to each microplate well. After another wash step, TMB-substrate solution is added to each well. Finally, a sulfuric acid stop solution is added and the resulting yellow colored product is measured at 450nm. The amount of sample IL-12p70 is determined by direct comparison with the standard curve generated in the assay.

Specifications:

Format:	1 X 96 well ELISA presented as 12 X 8 well (6 X 16 well) strips in frame.	
Number of tests:	Triplicate =	24
	Duplicate =	40
Specificity:	Human IL-12p70	
Sensitivity:	4.79 pg/mL	
Range:	4.79 pg/mL–500 pg/mL	

Kit Contents:

1 Foil Pouch	96 well microplate precoated with anti-Human IL-12p70	
2 bottles	20X Concentrated Wash Buffer	(25 mL)
1 vial	rHu IL-12p70 Standard (lyophilized)	(1 Vial)
1 bottle	Standard/Sample Dilution Buffer	(25mL)
1 vial	Secondary Antibody (Lyophilized) (Biotinylated Anti-Hu IL-12p70)	(1 Vial)
1 vial	100X Streptavidin-HRP Conjugate	(150 µL)
1 bottle	Reagent Dilution Buffer	(25mL)
1 bottle	TMB Substrate	(15 mL)
1 bottle	Stop Solution (1 N Sulfuric Acid, H ₂ SO ₄)	(15 mL)
2	Adhesive Plate Covers	(2)

Required Materials Not Provided:

Adjustable micropipettes with disposable tips (5-1000 µL). Multi-channel pipettes are useful and help to reduce intra-sample variability.

Polypropylene tubes.

Serological pipettes.

Deionized water.

Required Instrumentation:

Plate reader with **450 nm** capability (650 nm is required for optional monitoring of color development prior to stopping the reaction).

Warnings, Precautions & Limitations:

Reagents are intended for research use only and are not for use in diagnostic or therapeutic procedures.

Individual components may be harmful if swallowed, inhaled or absorbed through the skin. Contact should be minimized through the use of gloves and standard good laboratory practices. If contact with skin or eyes occurs, rinse the site immediately with water and consult a physician.

Substrate solutions must be at room temperature prior to use. Avoid contact of substrate solutions with oxidizing agents and metal.

Improper or insufficient washing at any stage of the procedure will result in either false positive or false negative results. Completely empty wells before dispensing fresh Wash Buffer, fill with Wash Buffer as indicated for each wash cycle and do not allow wells to sit uncovered or dry for extended periods.

Storage Instructions:

All kit components of this kit are stable at 2 to 8 °C. Any unused reconstituted standard should be discarded or frozen at -70 °C. Standard can be frozen and thawed one time only without loss of immunoreactivity.

Assay Preparation:

1. Determine the number of wells required to assay standards, samples and controls for the appropriate number of replicates. It is recommended that testing be performed in duplicate or triplicate if possible.
2. Create an assay template showing positioning of standards, controls and samples.
3. Bring all samples and reagents to room temperature before use.
4. To avoid condensation, do not open foil pouches containing the microtiter strips until after they have reached room temperature. Next remove the required number of strips and place in the frame supplied.

Return unused wells to the storage bag with desiccant, seal and store at 2-8 °C.

Reagent Preparation:*Secondary Antibody*

1. Reconstitute *Secondary Antibody* by adding 150 μL *Reagent Dilution Buffer* to the vial. Label as 100X Secondary Antibody.
2. Equilibrate 100X *Secondary Antibody* to room temperature, mix gently.
3. Mix 20 μL of 100X *Secondary Antibody* with 1.98 mL *Reagent Dilution Buffer* for each 16 well strip to be assayed. Label as **“Working Secondary Antibody ”**.
4. Return the unused reconstituted 100X *Secondary Antibody* to the refrigerator.

100X Streptavidin-HRP Conjugate

1. Equilibrate to room temperature, mix gently.
2. Mix 20 μL of 100X *Streptavidin-HRP Conjugate* with 1.98 mL *Reagent Dilution Buffer* for each 16-well strip to be assayed. Label as **“Working Streptavidin-HRP Conjugate”**.
3. Return the unused 100X *Streptavidin-HRP Conjugate* to the refrigerator.

Wash Buffer

1. Equilibrate to room temperature, mix to re-dissolve any precipitated salt.
2. Mix 0.5 volume 20X *Wash Buffer* with 9.5 volumes of *deionized water*. Label as **“Working Wash Solution”**.
3. Store both the remaining concentrated Wash Buffer and the Working Wash Solution at 4 °C in the refrigerator.

TMB Substrate

The TMB Substrate is provided ready to use.

Stop Solution

The Stop Solution is provided ready to use

Sample Handling/Preparation

The rate of degradation of human IL-12p70 in various matrices has not been fully investigated. It is beyond the scope of this publication to comment on specific sample processing protocols except to state that sodium citrate, heparin or EDTA are all acceptable forms of anticoagulant for use in harvesting plasma for this assay. It is also recommended that serum or plasma samples be centrifuged and separated from coagulated or packed cells as soon as possible after harvest. Serum and plasma samples should be diluted 20X prior to assay.

Cell lysates can be made by isolating cell samples followed by mechanical homogenization or sonication. Homogenates should be centrifuged and the assay performed on the clarified supernatant. Since the concentration of IL-12p70 in a cell or tissue homogenate will be highly dependent on type of cell or tissue it up to the end-user to optimize the dilutional scheme for their specific sample type.

Standard Curve Preparation:

Reconstitute the human IL-12p70 standard to 10 ng/mL by adding 1mL of *Standard/Sample Dilution Buffer* into the standard protein glass vial containing lyophilized human IL-12p70. Swirl or mix gently, and allow to sit for 5 minutes to ensure complete reconstitution. Use or freeze within 1 hour of reconstitution.

1. Label tubes 1-8 tubes as:
500, 250, 125, 62.5, 31.25, 15.63, 7.81 and zero (0) pg/mL.
2. Add 950 μ L *Standard/Sample Dilution Buffer* to tube 1 and 500 μ L *Standard/Sample Dilution Buffer* to each of tubes 2-8.
3. Add 50 μ L **Reconstituted 10 ng/mL Standard** to tube 1 and mix well.
Note: Unused reconstituted standard can be frozen at -70 °C and thawed one time only without significant loss of immunoreactivity.
4. Make a serial dilution by transferring 500 μ L of 500 pg/mL Standard (tube 1) into tube 2 mixing thoroughly then 500 μ L of resulting 250 pg/mL to tubes 3 and so on to create all Standards down to 7.81 pg/mL.


Assay Protocol:

1. Add 100 μL of **Diluted Standards** to the appropriate microtiter wells and 100 μL of **Standard/Sample Dilution Buffer** to zero wells.
 2. Add 100 μL of **Diluted (if necessary) Sample** to each well according to plan.
 3. Cover the plate with the plate cover and incubate for 2 hours at 37 °C.
 4. Thoroughly aspirate or decant the solution from the wells.
 5. Wash wells 3 times as follows: Dispense 300 μL **Working Wash Solution** to each well and allow to soak for 1-3 minutes before decanting or aspirating the remaining solution from the wells.
 6. Add 100 μL of **Working Secondary Antibody** to each well.
 7. Cover the plate with the plate cover and incubate for 1 hour at 37 °C.
 8. Aspirate or decant the solution from the wells then wash the wells 3 times as previously described in step 5.
 9. Add 100 μL **Working Streptavidin-HRP Conjugate** to each well.
 10. Cover the plate with the plate cover and incubate for 30 minutes at room temperature 37 °C.
 11. Thoroughly aspirate or decant the solution from the wells. Wash the wells 3 times previously described in step 5.
 12. Add 100 μL of **TMB Substrate** to each well. The highest standard wells and sample wells with high levels of IL-12p70 should begin to turn blue.
 13. Incubate the plate at room temperature for approximately 5-10 minutes. In some cases longer incubation may be necessary.
- Note: The incubation time for the TMB substrate is dependent on ambient conditions. The user can adjust this time as necessary by monitoring the development of blue color at 650 nm and applying stop solution when the high standard has reached near maximal absorbance level.
14. After appropriate incubation time, add 100 μL of **Stop Solution** to each well. The solution in the wells should change from blue to yellow.
 15. Read and record the absorbance of each well at 450 nm within 20

Data Analysis:

1. Plot the mean absorbance at 450 nm for each standard versus the IL-12p70 concentration. Select the best possible fit for the curve obtained. This can typically be done using the software provided with most plate readers. An example curve is shown below.
2. Sample IL-12p70 is determined by comparing their absorbance at 450 nm with those of the standard curve.
3. Sample data as read from the standard curve must be multiplied by the dilution factor used.

Note: Samples with an ABS_{450} exceeding that of the highest standard should be additionally diluted with Sample Dilution Buffer and re-assayed in order to avoid erroneous results.

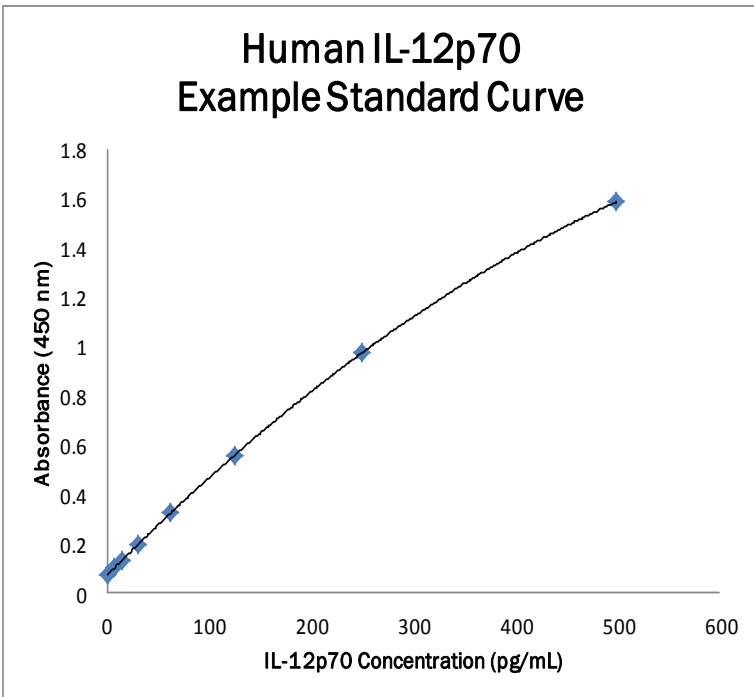

Performance Details:

The following substances were tested and found to have no crossreactivity:

Human IL-12p35	Human IL-12/IL-23p40
Human IL-23	Murine IL-12p70

Sensitivity

The lower limit of detection for human IL-12p70 in this assay was calculated by adding three standard deviations to the mean of 12 zero standard replicates and intersecting this value with the standard curve obtained in the same calculation. Sensitivity was calculated to be 4.79 pg/mL.

Precision

Intra-assay CV = 4.18 %

Inter-assay CV = 4.38 %

Accuracy:

Recovery on addition is 100~103% (Average 101.7%)


References:

1. Kunitaka, S. et al. (2000) *Br. J. Cancer*. 83, 928-934.
2. Strange, R. W. et al. (2003) *J. Mol. Biol.* 328, 877-891.
3. Weisiger, R. A., and Fridovich, I. (1973) *J. Biol. Chem.* 248, 3582-3592.
4. Enghild, J. J. et al. (1999) *Biochem J.* 317, 51-57.

Statement of Limited Warranty:

Northwest Life Science Specialties, LLC (NWLSS) makes no guarantee of any kind, expressed or implied, that extends beyond the description of the material in this kit, except that they will meet our specifications at the time of delivery. Customer's remedy and NWLSS' sole liability is limited to, at NWLSS' option, refund of the purchase price, or the replacement of material not meeting our specification. By acceptance of our product, customer assumes all liability and will indemnify and hold NWLSS harmless for the consequence of this product's use or misuse by the customer, its employees, or others. Refund or replacement is conditioned of customer notifying NWLSS within twenty-one (21) days of the receipt of product. Failure to give notice within 21 days shall constitute a waiver by the customer of all claims hereunder with respect to said product.

Notes:



Northwest

Life Science Specialties, LLC

5131 NE 94th Avenue, Suite 201

Vancouver, WA 98662

Phone 360-449-3091 or Toll Free: 888-449-3091

Fax 360-449-3092

E-mail: sales@nwlifescience.com